

(FOR RESEARCH USE ONLY. DO NOT USE IT IN CLINICAL DIAGNOSIS !)

Catalog No: E-BC-K083-M

Specification: 96T(40 samples)

Measuring instrument: Microplate reader (440-460 nm)

Detection range: 8.3-42.3 U/L

**Elabscience[®] α -Ketoglutarate Dehydrogenase(α -KGDH)
Activity Assay Kit**

This manual must be read attentively and completely before using this product.
If you have any problem, please contact our Technical Service Center for help:

Toll-free: 1-888-852-8623

Tell: 1-832-243-6086

Fax: 1-832-243-6017

Email: techsupport@elabscience.com


Website: www.elabscience.com

Please kindly provide us the lot number (on the outside of the box) of the kit for more efficient service.

Table of contents

Assay summary	3
Intended use	4
Detection principle	4
Kit components & storage	4
Materials prepared by users	5
Reagent preparation	5
Sample preparation	6
The key points of the assay	7
Operating steps	7
Calculation	8
Appendix I Performance Characteristics	9
Appendix II Example Analysis	11
Statement	12

Assay summary

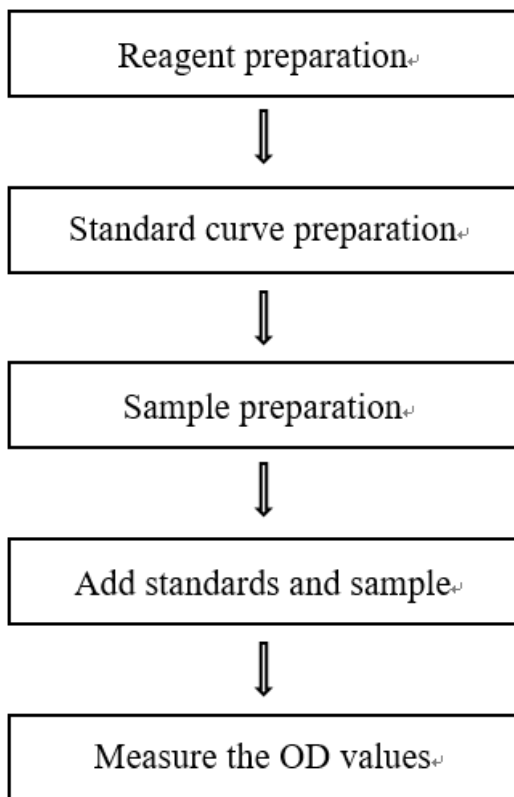

Intended use

This kit can measure α -ketoglutarate dehydrogenase (α -KGDH) activity in serum, plasma, animal and plant tissue samples.

Detection principle

α -ketoglutarate dehydrogenase (α -KGDH) is a key enzyme in the tricarboxylic acid (TCA) cycle. While the substrate being catalyzed by α -KGDH, NAD⁺ is reduced to NADH, and electrons are transferred to WST-8 under the action of hydrogen transmitter to produce yellow product. The activity of α -KGDH can be calculated by measuring the change of absorbance value at 450 nm.

Kit components & storage

Item	Component	Size 1(96 T)	Storage
Reagent 1	Extraction Solution	55 mL \times 1 vial	-20°C, 12 months
Reagent 2	Buffer Solution	28 mL \times 1 vial	-20°C, 12 months
Reagent 3	Substrate	Powder \times 1 vial	-20 °C, 12 months, shading light
Reagent 4	Chromogenic Agent	3 mL \times 1 vial	-20 °C, 12 months, shading light
Reagent 5	Clarificant	3mL \times 1 vial	-20°C, 12 months
Reagent 6	Standard	Powder \times 1 vial	-20°C, 12 months
	Microplate	96 wells	No requirement
	Plate Sealer	2 pieces	

Note: The reagents must be stored strictly according to the preservation conditions in the above table. The reagents in different kits cannot be mixed with each other. For a small volume of reagents, please centrifuge before use, so as not to obtain sufficient amount of reagents.

Materials prepared by users

Instruments:

Incubator, Centrifuge, Microplate reader (440-460 nm, optimum wavelength: 450 nm)

Reagent preparation

① Equilibrate all reagents to room temperature before use.

② The preparation of working solution :

Dissolve one vial of buffer solution with one vial of substrate, mix well to dissolve. Store at 2-8 °C for 6 h protected from light.

③ The preparation of 0.5 mmol/L standard solution :

Dissolve one vial of standard with 2 mL of double distilled water, mix well to dissolve. Store at 2-8 °C for 6 h protected from light.

④ The preparation of standard curve :

Always prepare a fresh set of standards. Discard working standard dilutions after use.

Dilute 0.5 mmol/L standard solution with double distilled water to a serial concentration. The recommended dilution gradient is as follows: 0, 0.1, 0.2, 0.25, 0.3, 0.35, 0.4, 0.5 mmol/L. Reference is as follows:

Item	①	②	③	④	⑤	⑥	⑦	⑧
Concentration (mmol/L)	0	0.1	0.2	0.25	0.3	0.35	0.4	0.5
0.5 mmol/L standard (μL)	0	40	80	100	120	140	160	200
Double distilled water (μL)	200	160	120	100	80	60	40	0

Sample preparation

① Sample preparation

Serum and plasma: detect directly. If not detected on the same day, the serum or plasma can be stored at -80°C for a month.

Tissue sample:

- ① Harvest the amount of tissue needed for each assay (initial recommendation 20 mg).
- ② Wash tissue in cold PBS (0.01 M, pH 7.4).
- ③ Homogenize 20 mg tissue in 180 μL extraction solution with a dounce homogenizer at 4°C.
- ④ Centrifuge at 10000 \times g for 10 minutes at 4°C to remove insoluble material. Collect supernatant and keep it on ice for detection.
- ⑤ Meanwhile, determine the protein concentration of supernatant (E-BC-K318-M).

② Dilution of sample

The recommended dilution factor for different samples is as follows (for reference only):

Sample type	Dilution factor
10% Rat liver tissue homogenate	1
10% Rat lung tissue homogenate	1
10% Mouse liver tissue homogenate	1
10% <i>Epipremnum aureum</i> tissue homogenate	1
10% Mouse spleen tissue homogenate	1
Rat plasma	1

Note: The diluent is extraction solution. For the dilution of other sample types, please do pretest to confirm the dilution factor

The key points of the assay

The powder must be completely dissolved while preparing the working solution.

Operating steps

- ① Standard well: Add 20 μL of standard solution with different concentrations to the corresponding wells.
Sample well: Add 20 μL of sample to the corresponding wells.
Control well: Add 20 μL of sample to the corresponding wells
- ② Add 200 μL of working solution to standard well and sample well. Add 200 μL of double distilled water to control well
- ③ Add 20 μL of chromogenic agent to each well.
- ④ Mix fully with microplate reader for 3 s, incubate at 37 $^{\circ}\text{C}$ for 10 min with shading light.
- ⑤ Add 20 μL of clarificant to each well.
- ⑥ Mix fully with microplate reader for 3 s, and measure the OD value of each well at 450 nm with microplate reader.

Calculation

The standard curve:

1. Average the duplicate reading for each standard.
2. Subtract the mean OD value of the blank (Standard #①) from all standard readings. This is the absolved OD value.
3. Plot the standard curve by using absolved OD value of standard and correspondent concentration as y-axis and x-axis respectively. Create the standard curve ($y = ax + b$) with graph software (or EXCEL).

The sample:

1. Serum (plasma) sample:

Definition: The amount of α -KGDH in 1 L serum (plasma) per 1 minute that hydrolyze the substrate to produce 1 μ mol NADH at 37°C is defined as 1 unit.

$$\alpha\text{-KGDH activity (U/L)} = (\Delta A_{450} - b) \div a \div T \times 1000 \times f$$

2. Tissue sample:

Definition: The amount of α -KGDH in 1 g tissue protein per 1 minute that hydrolyze the substrate to produce 1 μ mol NADH at 37 °C is defined as 1 unit

$$\alpha\text{-KGDH activity (U/gprot)} = (\Delta A_{450} - b) \div a \div T \times 1000 \div C_{pr} \times f$$

[Note]

ΔA_{450} : $OD_{\text{Sample}} - OD_{\text{Control}}$.

T: The time of reaction, 10 min.

C_{pr} : The concentration of protein in sample, gprot/L.

f: Dilution factor of sample before test.

1000*: 1 mmol = 1000 μ mol.

Appendix I Performance Characteristics

1. Parameter:

Intra-assay Precision

Three human serum samples were assayed in replicates of 20 to determine precision within an assay (CV = Coefficient of Variation).

Parameters	Sample 1	Sample 2	Sample 3
Mean (U/L)	12.50	27.60	33.80
%CV	1.7	1.4	1.4

Inter-assay Precision

Three human serum samples were assayed 20 times in duplicate by three operators to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3
Mean (U/L)	12.50	27.60	33.80
%CV	8.2	8.5	8.8

Recovery

Take three samples of high concentration, middle concentration and low concentration to test the samples of each concentration for 6 times parallelly to get the average recovery rate of 100%.

	Standard 1	Standard 2	Standard 3
Expected Conc. (mmol/L)	0.15	0.28	0.37
Observed Conc. (mmol/L)	0.2	0.3	0.4
recovery rate(%)	101	98	101


Sensitivity

The analytical sensitivity of the assay is 8.3 U/L. This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 20 times, and calculating the corresponding concentration.

2. Standard curve:

As the OD value of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique or temperature effects), so the standard curve and data are provided as below for reference only:

Concentration (mmol/L)	0	0.1	0.2	0.25	0.3	0.35	0.4	0.5
Average OD	0.091	0.238	0.436	0.545	0.601	0.681	0.811	1.017
Absoluted OD	0	0.147	0.345	0.453	0.509	0.589	0.719	0.925

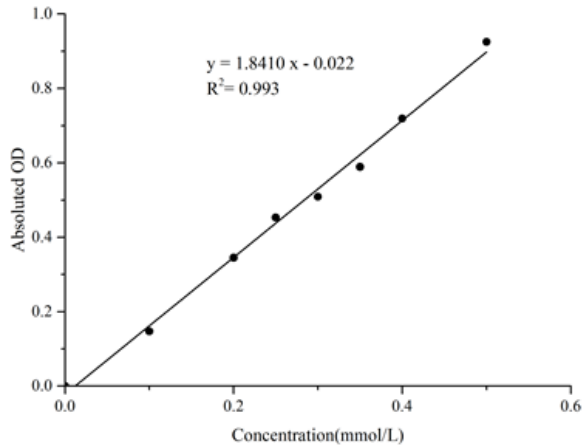

Appendix II Example Analysis


Example analysis:

For mouse liver tissue, take 20 μL of 10% mouse liver tissue homogenate, and carry the assay according to the operation steps. The results are as follows:

standard curve: $y = 1.7013x - 0.0006$, the average OD value of the control is 0.113, the average OD value of the sample is 0.397, the concentration of protein in sample is 13.89 gprot/L, and the calculation result is:

$$\begin{aligned}\alpha\text{-KGDH activity (U/gprot)} &= (0.397 - 0.113 + 0.0006) \div 1.7013 \div 10 \times 1000 \div 13.89 \\ &= 1.20 \text{ U/gprot}\end{aligned}$$

Detect 10% mouse liver tissue homogenate (the concentration of protein is 13.89 gprot/L), 10% *Epipremnum aureum* tissue homogenate (the concentration of protein is 3.63 gprot/L), rat plasma and mouse plasma according to the protocol, the result is as follows:

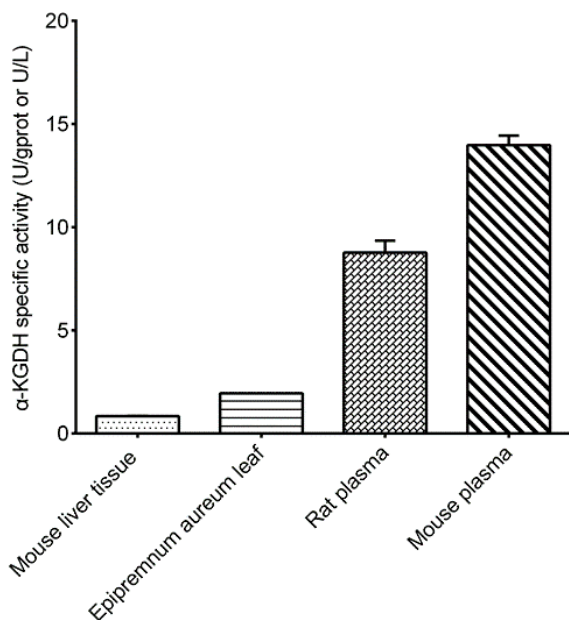

Statement

1. This assay kit is for Research Use Only. We will not response for any arising problems or legal responsibilities causing by using the kit for clinical diagnosis or other purpose.
2. Please read the instructions carefully and adjust the instruments before the experiments. Please follow the instructions strictly during the experiments.
3. Protection methods must be taken by wearing lab coat and latex gloves.
4. If the concentration of substance is not within the detection range exactly, an extra dilution or concentration should be taken for the sample.
5. It is recommended to take a pre-test if your sample is not listed in the instruction book.
6. The experimental results are closely related to the situation of reagents, operations, environment and so on. Elabscience will guarantee the quality of the kits only, and NOT be responsible for the sample consumption caused by using the assay kits. It is better to calculate the possible usage of sample and reserve sufficient samples before use.