

(FOR RESEARCH USE ONLY. DO NOT USE IT IN CLINICAL DIAGNOSIS !)

**Catalog No: E-BC-K234-M**

**Specification: 48T(32 samples)/96T(80 samples)**

**Measuring instrument: Microplate reader (500-510 nm)**

**Detection range: 0.04-30 mmol/L**

**Elabscience<sup>®</sup> Glucose (Glu) Colorimetric Assay Kit**  
**(GOD-POD Method)**

This manual must be read attentively and completely before using this product.  
If you have any problem, please contact our Technical Service Center for help:

Toll-free: 1-888-852-8623

Tell: 1-832-243-6086

Fax: 1-832-243-6017

Email: [techsupport@elabscience.com](mailto:techsupport@elabscience.com)


Website: [www.elabscience.com](http://www.elabscience.com)

Please kindly provide us the lot number (on the outside of the box) of the kit for more efficient service.

## Table of contents

<b>Assay summary</b> .....	3
<b>Intended use</b> .....	4
<b>Detection principle</b> .....	4
<b>Kit components &amp; storage</b> .....	4
<b>Materials prepared by users</b> .....	5
<b>Reagent preparation</b> .....	5
<b>Sample preparation</b> .....	6
<b>The key points of the assay</b> .....	7
<b>Operating steps</b> .....	7
<b>Calculation</b> .....	8
<b>Appendix I Performance Characteristics</b> .....	9
<b>Appendix II Example Analysis</b> .....	11
<b>Statement</b> .....	12

## Assay summary

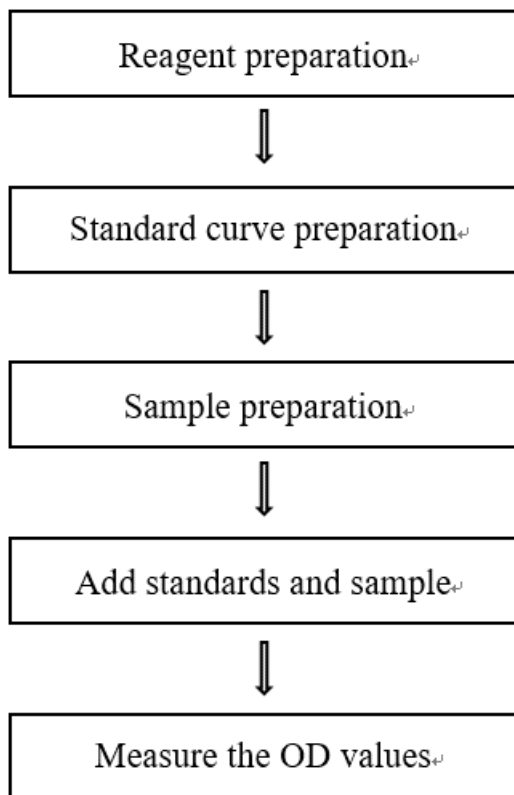

## Intended use

This kit can be used to measure the Glucose (Glu) content in whole blood, serum, plasma samples.

## Detection principle

Glucose oxidase can catalyze the oxidation of glucose to gluconic acid to produce hydrogen peroxide. In the presence of chromogenic oxygen receptors, peroxidase catalyzes hydrogen peroxide and oxidizes pigment sources to form colored substances. Measure the OD value at 505 nm and glucose content can be calculated indirectly.

## Kit components & storage

Item	Component	Size 1(48 T)	Size 2(96 T)	Storage
Reagent 1	Phenol Solution	10 mL × 1 vial	20 mL × 1 vial	2-8 °C, 12 months shading light
Reagent 2	Enzyme Solution	10 mL × 1 vial	20 mL × 1 vial	2-8 °C, 12 months shading light
Reagent 3	50 mmol/L Glucose Standard	1.2 mL × 1 vial	1.2 mL × 1 vial	2-8 °C, 12 months
	Microplate	96 wells		No requirement
	Plate Sealer	2 pieces		

Note: The reagents must be stored strictly according to the preservation conditions in the above table. The reagents in different kits cannot be mixed with each other. For a small volume of reagents, please centrifuge before use, so as not to obtain sufficient amount of reagents.

## Materials prepared by users

### Instruments:

Microplate reader (500-510 nm), Vortex mixer, Micropipettor, Incubator

### Reagents:

Double distilled water, Normal saline (0.9% NaCl)

## Reagent preparation

① Equilibrate all reagents to room temperature before use.

② The preparation of enzyme working solution:

For each well, prepare 300  $\mu\text{L}$  of enzyme working solution (mix well 150  $\mu\text{L}$  of phenol solution and 150  $\mu\text{L}$  of enzyme solution). The enzyme working solution should be prepared on spot. Store at 2-8  $^{\circ}\text{C}$  for 24 h protected from light.

③ The preparation of control working solution:

For each well, prepare 300  $\mu\text{L}$  of control working solution (mix well 150  $\mu\text{L}$  of normal saline and 150  $\mu\text{L}$  of enzyme solution). The control working solution should be prepared on spot. Store at 2-8  $^{\circ}\text{C}$  for 24 h protected from light.

④ The preparation of standard curve:

Always prepare a fresh set of standards. Discard working standard dilutions after use.

Dilute 50 mmol/L glucose standard with double distilled water to a serial concentration. The recommended dilution gradient is as follows: 0, 2, 5, 10, 15, 20, 25, 30 mmol/L. Reference is as follows:

Item	①	②	③	④	⑤	⑥	⑦	⑧
<b>Concentration (mmol/L)</b>	<b>0</b>	<b>2</b>	<b>5</b>	<b>10</b>	<b>15</b>	<b>20</b>	<b>25</b>	<b>30</b>
<b>50 mmol/L glucose standard (<math>\mu\text{L}</math>)</b>	0	4	10	20	30	40	50	60
<b>Double distilled water (<math>\mu\text{L}</math>)</b>	100	96	90	80	70	60	50	40

## Sample preparation

### ① Sample preparation

**Serum, plasma and whole blood:** detect directly. If not detected on the same day, the serum or plasma can be stored at -80 °C for a month.

### ② Dilution of sample

The recommended dilution factor for different samples is as follows (for reference only):

Sample type	Dilution factor
Human serum	1
Mouse serum	1
Rat serum	1
Human plasma	1

Note: The diluent is normal saline (0.9% NaCl). For the dilution of other sample types, please do pretest to confirm the dilution factor

## The key points of the assay

- ① Set control wells for whole blood, hemolysis serum and plasma samples, but not for normal serum and plasma.
- ② To avoid contamination, do not put the pipette directly into the reagent bottle when using enzyme solution.

## Operating steps

- ① Standard well: Take 3  $\mu\text{L}$  of standard solution with different concentration to the wells.  
Sample well: Take 3  $\mu\text{L}$  of sample to the wells.  
Control well: Take 3  $\mu\text{L}$  of sample to the wells.
- ② Add 300  $\mu\text{L}$  of enzyme working solution into the standard and sample well.  
Add 300  $\mu\text{L}$  of control working solution into the control well.
- ③ Cover the plate sealer and incubate at 37  $^{\circ}\text{C}$  for 15 min.
- ④ Measure the OD value of each well with microplate reader at 505 nm.

**Note: Set control wells for whole blood, hemolysis serum and plasma samples, but not for normal serum and plasma.**

## Calculation

### The standard curve:

1. Average the duplicate reading for each standard.
2. Subtract the mean OD value of the blank (Standard #①) from all standard readings. This is the absolved OD value.
3. Plot the standard curve by using absolved OD value of standard and correspondent concentration as y-axis and x-axis respectively. Create the standard curve ( $y = ax + b$ ) with graph software (or EXCEL).

### The sample:

#### 1. Normal serum (plasma) sample:

$$\text{Glu content (mmol/L)} = (\Delta A_{505} - b) \div a \times f$$

#### 2. Whole blood and hemolysis sample:

$$\text{Glu content (mmol/L)} = (\Delta A' - b) \div a \times f$$

[Note]

$\Delta A_{505}$ :  $OD_{\text{Sample}} - OD_{\text{Blank}}$ .

$\Delta A'$ :  $OD_{\text{Sample}} - OD_{\text{Control}}$ .

f: Dilution factor of sample before tested.



## Appendix I Performance Characteristics

### 1. Parameter:

#### Intra-assay Precision

Three human serum samples were assayed in replicates of 20 to determine precision within an assay. (CV = Coefficient of Variation)

Parameters	Sample 1	Sample 2	Sample 3
Mean (mmol/L)	1.50	13.40	25.50
%CV	2.4	2.1	1.2

#### Inter-assay Precision

Three human serum samples were assayed 20 times in duplicate by three operators to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3
Mean (mmol/L)	1.50	13.40	25.50
%CV	2.5	1.7	2.7

#### Recovery

Take three samples of high concentration, middle concentration and low concentration to test the samples of each concentration for 6 times parallelly to get the average recovery rate of 100%.

	Standard 1	Standard 2	Standard 3
Expected Conc. (mmol/L)	3.6	11.5	24.5
Observed Conc. (mmol/L)	3.6	11.4	24.5
recovery rate(%)	101	99	100


#### Sensitivity

The analytical sensitivity of the assay is 0.04 mmol/L. This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 20 times, and calculating the corresponding concentration.

## 2. Standard curve:

As the OD value of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique or temperature effects), so the standard curve and data are provided as below for reference only:

Concentration (mmol/L)	0	2	5	10	15	20	25	30
Average OD	0.043	0.152	0.318	0.583	0.863	1.148	1.406	1.647
Absoluted OD	0	0.110	0.276	0.540	0.820	1.106	1.363	1.604

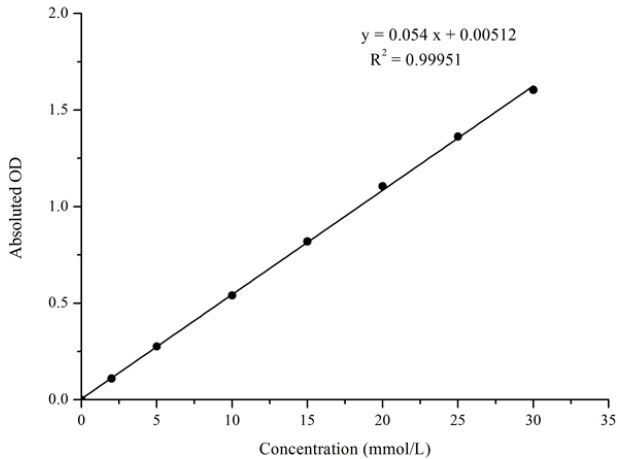

## Appendix II Example Analysis


### Example analysis:

Take 3  $\mu\text{L}$  of mouse serum, carry the assay according to the operation steps. The results are as follows:

standard curve:  $y = 0.054x + 0.00512$ , the average OD value of the sample is 0.327, the average OD value of the blank is 0.043, and the calculation result is:

$$\text{Glu content (mmol/L)} = (0.327 - 0.043 - 0.00512) \div 0.054 = 5.17 \text{ (mmol/L)}$$

Detect mouse serum, rat plasma, according to the protocol, the result is as follows:

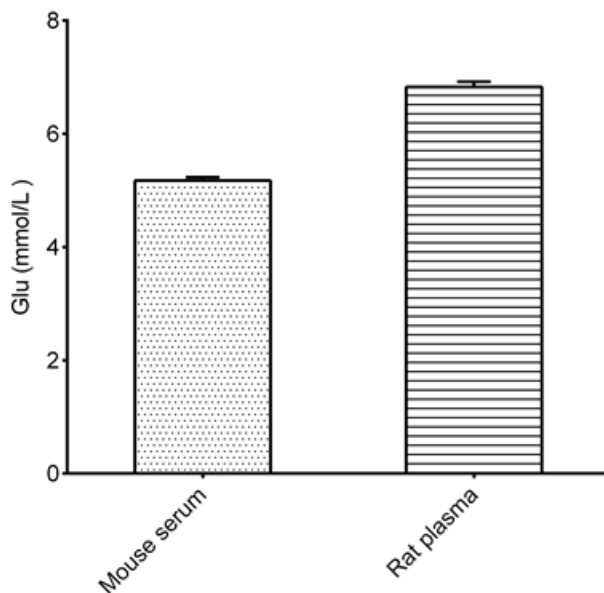

## Statement

1. This assay kit is for Research Use Only. We will not response for any arising problems or legal responsibilities causing by using the kit for clinical diagnosis or other purpose.
2. Please read the instructions carefully and adjust the instruments before the experiments. Please follow the instructions strictly during the experiments.
3. Protection methods must be taken by wearing lab coat and latex gloves.
4. If the concentration of substance is not within the detection range exactly, an extra dilution or concentration should be taken for the sample.
5. It is recommended to take a pre-test if your sample is not listed in the instruction book.
6. The experimental results are closely related to the situation of reagents, operations, environment and so on. Elabscience will guarantee the quality of the kits only, and NOT be responsible for the sample consumption caused by using the assay kits. It is better to calculate the possible usage of sample and reserve sufficient samples before use.